


-15kV TOF: -9051 v  
 -3.6kV MCP: -2688 v  
 -2.4kV MCP: -1640 v  
 Input Cur: 306 ma  
 RPA max: 235 v  
 Mirror max: 238 v

Tue Sep 26 12:15:07 2006

## TIDE Direct Events

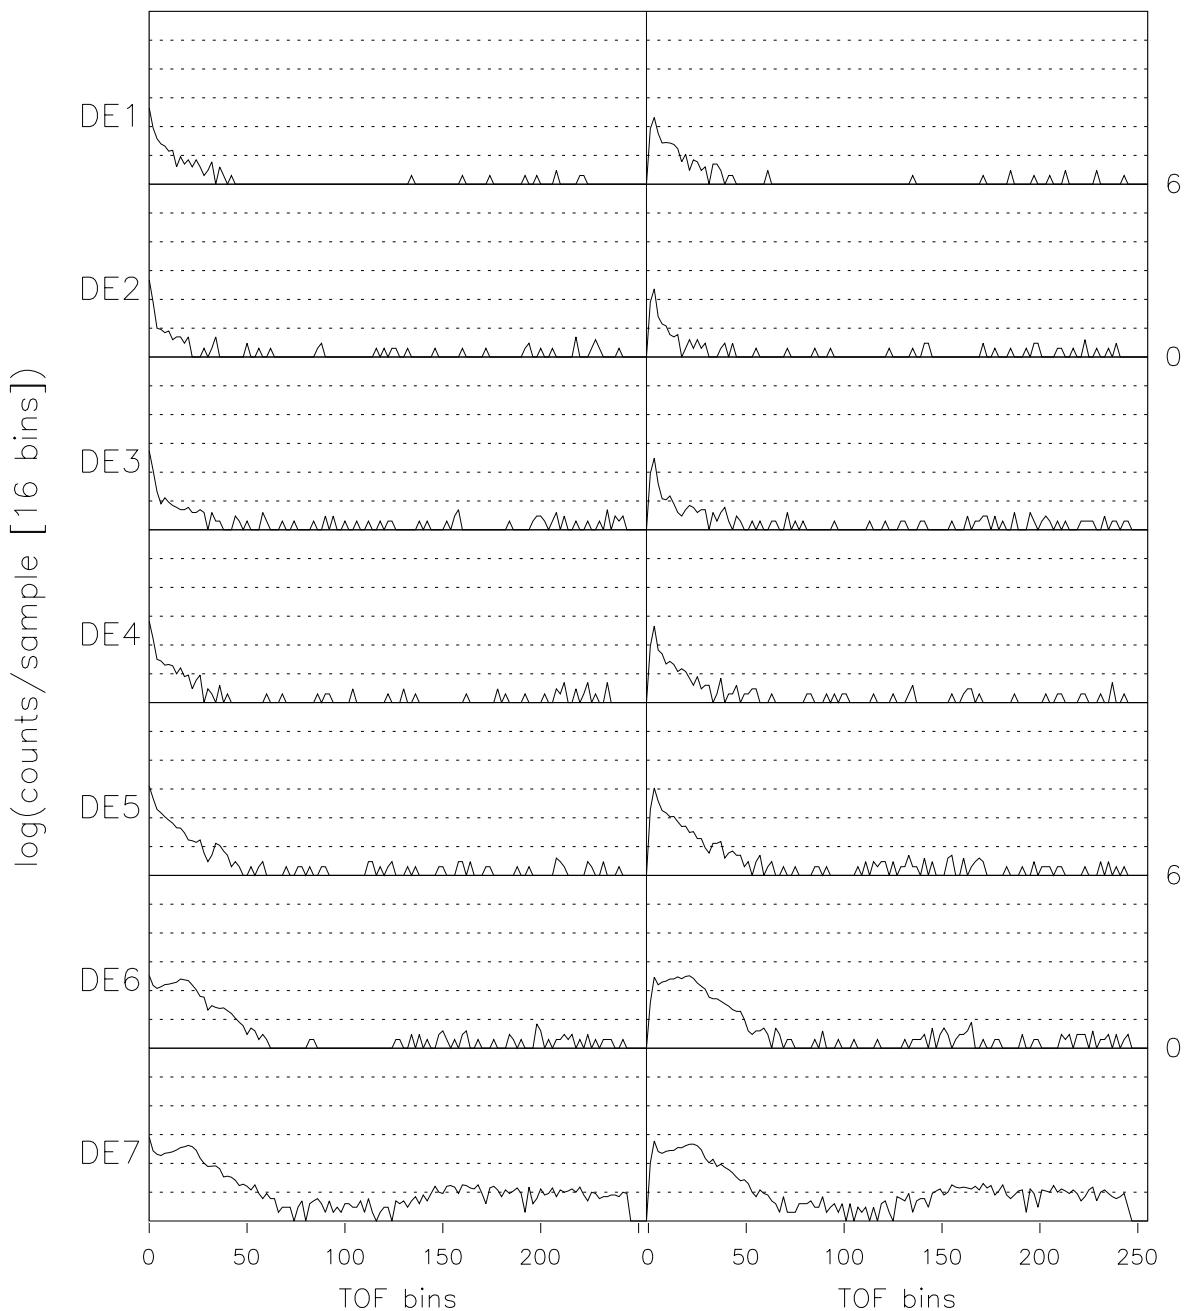

reported: 08-23-96 19:57:53 UT

reported: 08-23-96 20:01:04 UT

file: /export/data/tide/nrt/96082301.dat

-15kV TOF: -9051 v

-3.6kV MCP: -2672 v

-2.4kV MCP: -1640 v

Input Cur: 306 ma

RPA max: 236 v

Mirror max: 238 v